


Nitrile Examination Powder Free Glove

EN 420:2003 + A1:2009

Fit For Special Purpose (Palm protection)

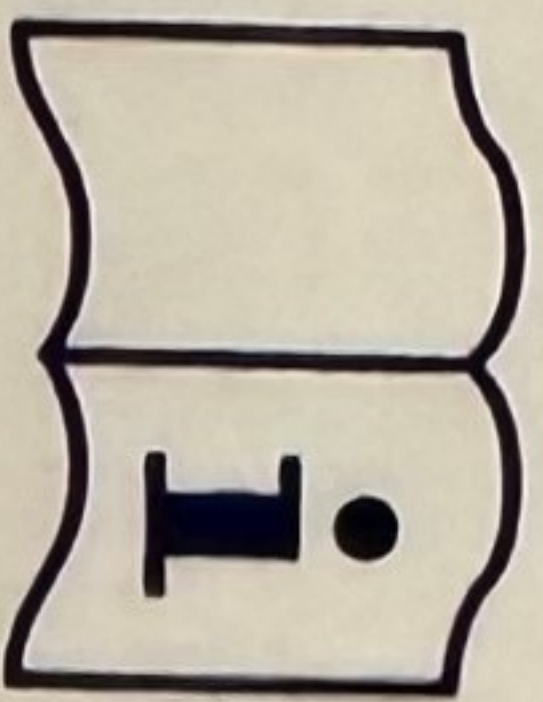

are worn on the hands of the healthcare and similar personnel to prevent contamination between healthcare personnel and patient /user"

EU Type Examination and ongoing Conformity

by Notified Body: **Satra Technology Europe LTD**

Bracetown Business Park, Clonee D15 YN2P, Ireland.

Resistance against Bacteria and Fungi - **PASS**

Resistance against Virus - **PASS**



This is a Medical Device

EN ISO 374-1:2016 Classification of P

Measured Breakthrough time (min)	
> 10	
> 30	
> 60	
> 120	
> 240	
> 480	

REP
Representative
an Community



Lotus NL B.V.
Koningin Julianaplein 10,
1e Verd, 2595 AA, The Hague,
The Netherlands



Comply to MDR 2017/745 Class I
2777 Comply to PPE Regulation 2016/425 Cat III

Hand Size	6 (XS)	7 (S)
Min Length	240mm	240mm

EN ISO 374-1:2016/type B

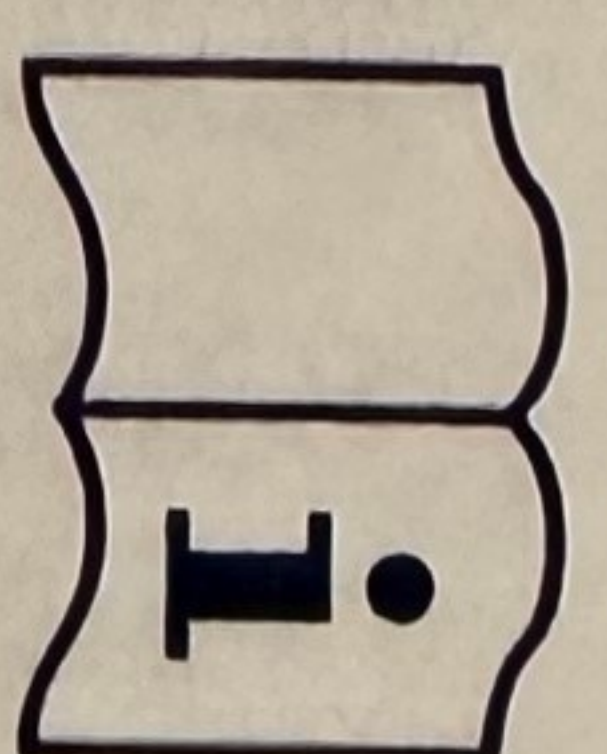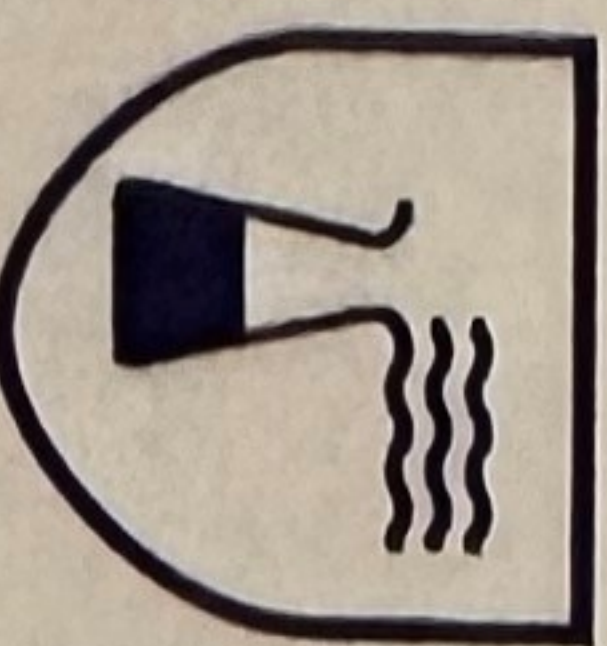

KPT



Manufacturer:

Blue Sail Medical Co., Ltd
No. 21 Qingtian Road, Qilu
Chemical Industrial Park,
Zibo, Shandong 255414 China

Code letter	Chemical Permeation (EN ISO 374-1:2016)	Level	Mean Deg	Deg char the cher
K	40% Sodium Hydroxide	6	-38,4%	
P	30% Hydrogen Peroxide	2	17,60%	
T	37% Formaldehyde	5	46,6%	