
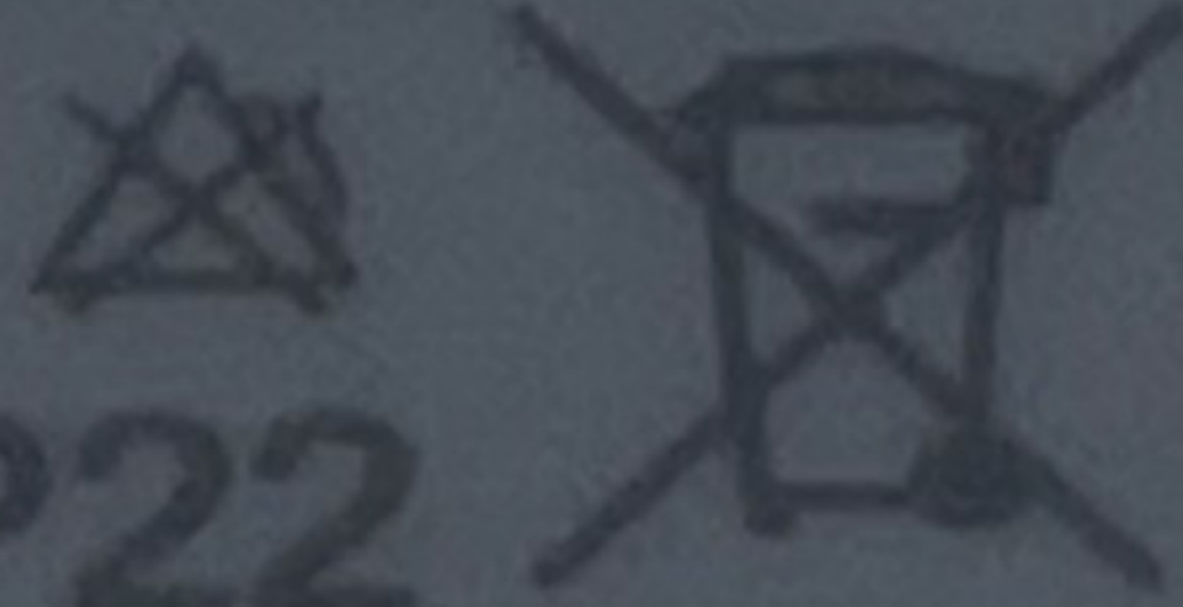



CONTEC Pulse Oximeter

Model: CMS50D2
Battery Voltage: DC 2.6 V-3.6 V
Operating Current: ≤ 80 mA
Safety Class: Type BF 



IP22

 Contec Medical Systems Co., Ltd.
No. 112 Qinhuang West Street,
Qinhuangdao,
Hebei Province, P.R.China


 0123

OPEN 

Shanghai International Holding Corp.GmbH(Europe)
Eilbeistrasse 80,20537 Hamburg,Germany

 See SN Code


2022-08

