

Dr. pen  [®]
Auto Microneedle System: 



User Manual *M8S*

Please read the manual before use




Product description	2
Parts name	3
Introduction for wireless mode	4
How to charge the battery	4
How to apply the needle cartridge	5
Adjustment of needle length	6
Speed display and adjustment	6
Needle cartridge introduction	7
Reference chart	8
Specification	8
Precaution	9
Warranty	10



The device consists of an electric microneedling pen and disposable needle cartridges. This manual will explain how to use each component in detail.

The device is used to improve the appearance of the skin and reduce signs of aging. It is intended to stimulate the skin with micro-needles for collagen and elastin production. The microchannels created in the superficial skin by the device also help with the absorption of skin serums.

There are 7 different types of needle cartridges designed for the device. These cartridges can be used for micro-needling treatment and nano-needling treatment.

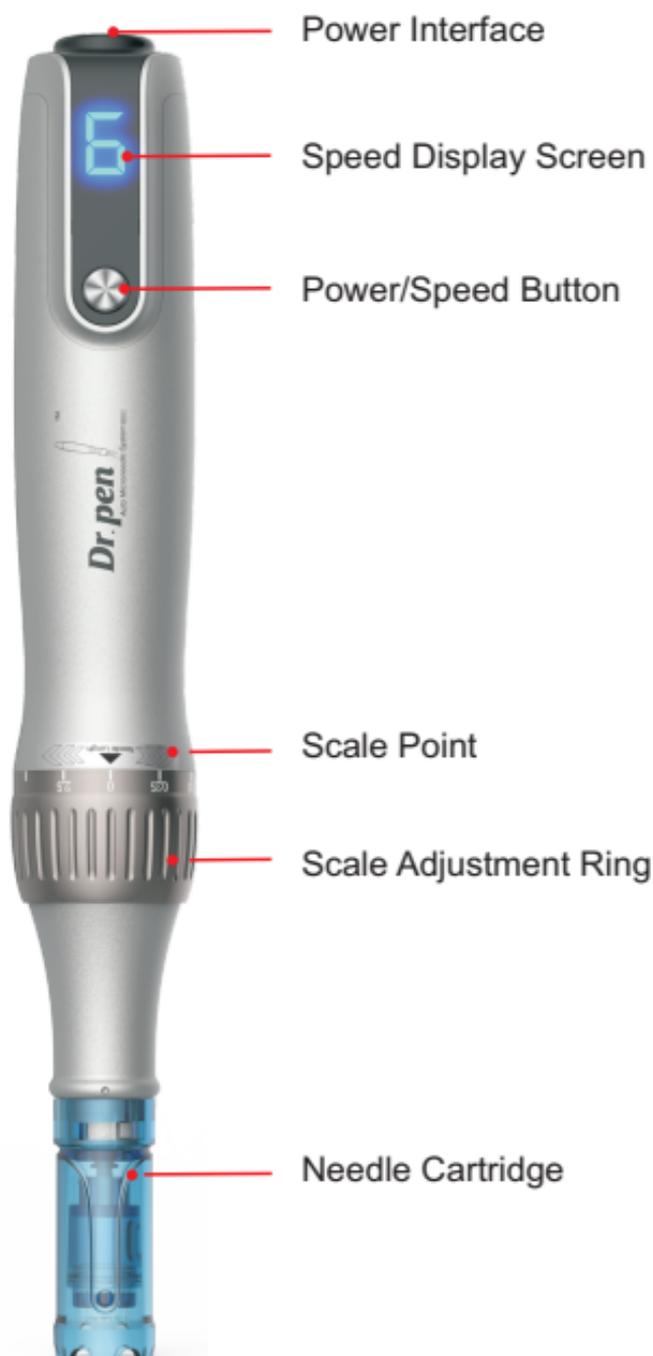



Introduction for wireless mode 4

This device is powered by a built-in battery. It can work wirelessly. The power cable and the adapter are used to charge the device when it is out of battery.



How to charge the battery

Connect the device to the adapter with the power cable, and plug the adapter into a live AC outlet to charge the device. Charging will be completed within 2 hours.

Charging Status

The number of speed flashes slowly when the battery capacity 10% left .

The pen turn off automatically after 1 minute while the number of speed flashes quickly .



Please charge the battery

when the pen show “



”

The pen show spinning “



”

The pen show “




”

when charging is completed.




Preparation

1. Take out needle cartridge from the sterilized packaging. [Fig1]

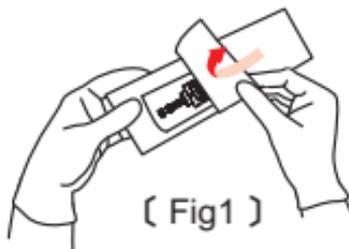

2. Find the "U" shape notch on the cartridge, align the notch with the dot on the bottom of the device, and slightly push the cartridge into the device. [Fig2]

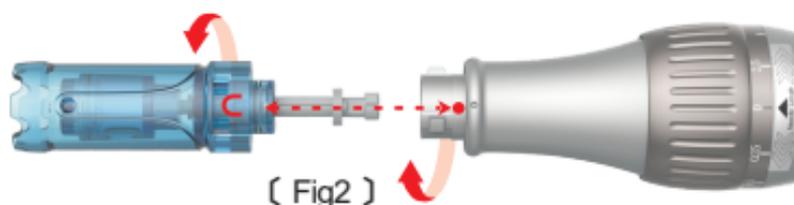

3. Lock the needle cartridge to the device by turning it clockwise.
4. Turn the needle cartridge counterclockwise and pull it out when you would like to remove the cartridge.
5. Start the device only when the needle cartridge is assembled correctly. Press and hold the power button for 3 seconds to turn on/off the device.

Before assembling or disassembling the needle cartridge, make sure the U-shaped point of the needle cartridge is aligned with the point of the handpiece.

The needle cartridge is designed for single use.

Place the used needle cartridges in a trash container. If the needle cartridge is inadvertently contaminated during installation (i.e. Dropped on the floor, package opened/damaged. The needle cartridge may be contaminated.), Please discard it and get a new needle cartridge.



Adjustment of needle length

6

Use suitable needle size according to different treatment areas and skin problems

Adjust the depth of the needle by turning the scale adjustment ring. The depth of the needle should be adjusted after starting the pen. The scale number aligning with the scale point shows the current needle depth. [Fig3]



Speed display and adjustment

Speed Display



6 Speed Adjustment

Press and hold the power button for 3 seconds to start or shut down the device. After starting the device, the speed changes once every time the power button is pressed.



Available needle cartridges



12 Needles



24 Needles



36 Needles



42 Needles



R NANO
Needles



S NANO
Needles



18 Needles



Attention

The needle cartridge is designed for Dr.pen M8S only.
The needle cartridge is disposable.

Please sterilize the needle cartridge with 75% alcohol
for a few minutes before use.

Please dispose the used needle cartridge to the trash
container.





Reference chart

8

REGION	NEEDLE DEPTH (MM)
Forehead	0.25 - 0.5
Between the Eyebrows	0.25 - 0.5
Nose	0.25
Around the orbital rim	0.25
Cheek and Chin	0.5 - 1.0
Surgical and Scar Maximum	2.5



Specification

Product name:

Auto-stamp Motorized Meso Machine

Model name: Dr.pen M8S

Adapter

Input: 100-240V 50-60HZ

Output: 5V $\overline{\text{---}}$ 1A

Package Weight: 400 g

Package Size: 169*123*56 mm

Packing List

Item	Quantity
Hand Piece	1 pc
Adapter	1 pc
Manual	1 pc
Power Cable	1 pc
Needle Cartridge	2 pcs



	Please be sure to read the instructions before use and follow as described.		
	Do not apply it to the person as following: 1. Who has acute disease or bloody disease over 38°C 2. Who has allergy and hemophilia 3. Who has melanosis of the face 4. Who has high internal heat 5. Who regularly visits hospital 6. Who takes medicines 7. Who is under 12 years old		
	Do not use it on the power other than AC 220V. It may cause fires or malfunction.		
	Do not use it near the place with high temperature, dust or humidity (Near the humidifier). It may cause malfunction.		
	Do not repair, disassemble or alter the controller and the body. It may cause malfunction.		
	Do not touch the device or detach the power cords with wet hands. It may cause electric shock.		
	Do not use the stripped cord or propped cord. It may cause fires(Be sure to replace it with another).		
	Do not use the propped cord which has crack or scares. It may cause scares on the skin.		
	When you don't use it for a long time, unplug it from the outlet.		
	Be sure to have an inspection for test. If any troubles are found, get it repaired.		
	No one other than the operator can touch it. It may cause accidents or malfunction.		
	Alternating current		Serial No
	Direct current		CE mark
	Attention, consult accompanying documents		Manufacturer
	Date of manufacture		Consult instruction for use



The warranty period of the device is 12 months. We offer repair service from the purchase date. If any of our products has damages or natural trouble, we provide replacements or repair service. The use of third-party cartridges can cause damage to the device. This could invalidate the warranty.

General maintenance

Make sure to inspect the device and adapter before use.

Ensure the device is turned off when not in use. Wipe its surface with a disinfecting wipe.

Pay attention to clean areas such as crevices, seams, and areas around where the needle cartridge attaches to the device.

Keep it away from direct sunlight or high temperature or humidity.

Do not leave the measurement, repair or alter of the device to non-professional staffs.

When you use the device which has not been used for a long time, make sure to check if it works properly with safety.

Dr. pen  [®]

M8S USER MANUAL